

ISO/IEC 17025:1999  
ISO 9002:1994

## Scope of Accreditation



Revised 8/6/04

Page 1 of 5

### CALIBRATION LABORATORIES

NVLAP LAB CODE 200106-0

#### DENVER INSTRUMENT COMPANY ALSO DOING BUSINESS AS SARTORIUS CORP.

6542 Fig Street  
Arvada, CO 80004-1042  
Mr. Mark Fritz  
Phone: 303-403-4690 x192 Fax: 303-431-4540  
E-Mail: mark.fritz@denverinstrument.com

**NVLAP Code:** 20/A01

ANSI/NCSL Z540-1-1994; Part 1

Compliant

### MECHANICAL

**NVLAP Code:** 20/M08

Mass  
Metric

<i>Range</i>	<i>Best Uncertainty (<math>\pm</math>) in mg<sup>note 1</sup></i>	<i>Remarks</i>
10 kg	1.591	Echelon I
5 kg	0.815	Echelon I
4 kg	0.713	Echelon I
3 kg	0.523	Echelon I
2 kg	0.295	Echelon I
1 kg	0.076	Echelon I
500 g	0.045	Echelon I
400 g	0.038	Echelon I

December 31, 2004

Effective through

For the National Institute of Standards and Technology

ISO/IEC 17025:1999  
ISO 9002:1994

## Scope of Accreditation



Revised 8/6/04

Page 2 of 5

### CALIBRATION LABORATORIES

NVLAP LAB CODE 200106-0

### DENVER INSTRUMENT COMPANY ALSO DOING BUSINESS AS SARTORIUS CORP.

300 g	0.034	Echelon I
200 g	0.028	Echelon I
100 g	0.0163	Echelon I
50 g	0.0097	Echelon I
30 g	0.0088	Echelon I
20 g	0.0083	Echelon I
10 g	0.0066	Echelon I
5 g	0.0049	Echelon I
3 g	0.0043	Echelon I
2 g	0.0039	Echelon I
1 g	0.0032	Echelon I
500 mg	0.00119	Echelon I
300 mg	0.00119	Echelon I
200 mg	0.00119	Echelon I
100 mg	0.00119	Echelon I
50 mg	0.00119	Echelon I

December 31, 2004

Effective through



For the National Institute of Standards and Technology

ISO/IEC 17025:1999  
ISO 9002:1994

## Scope of Accreditation



Revised 8/6/04

Page 3 of 5

### CALIBRATION LABORATORIES

NVLAP LAB CODE 200106-0

**DENVER INSTRUMENT COMPANY ALSO DOING BUSINESS AS SARTORIUS CORP.**

30 mg	0.00081	Echelon I
20 mg	0.00081	Echelon I
10 mg	0.00065	Echelon I
5 mg	0.00065	Echelon I
3 mg	0.00065	Echelon I
2 mg	0.00065	Echelon I
1 mg	0.00065	Echelon I
0.5 mg	0.00065	Echelon I

*NVLAP Code:* 20/M08  
Avoirdupois

<i>Range</i>	<i>Best Uncertainty (<math>\pm</math>) in mg<sup>note 1</sup></i>	<i>Remarks</i>
20 lb	1.75	Echelon I
10 lb	0.98	Echelon I
5 lb	0.26	Echelon I
3 lb	0.26	Echelon I
2 lb	0.24	Echelon I
1 lb	0.068	Echelon I

December 31, 2004

Effective through

For the National Institute of Standards and Technology

ISO/IEC 17025:1999  
ISO 9002:1994

## Scope of Accreditation



Revised 8/6/04

Page 4 of 5


### CALIBRATION LABORATORIES

NVLAP LAB CODE 200106-0

**DENVER INSTRUMENT COMPANY ALSO DOING BUSINESS AS SARTORIUS CORP.**

0.5 lb	0.055	Echelon I
0.3 lb	0.037	Echelon I
0.2 lb	0.034	Echelon I
0.1 lb	0.0149	Echelon I
0.05 lb	0.0068	Echelon I
0.03 lb	0.0065	Echelon I
0.02 lb	0.0065	Echelon I
0.01 lb	0.0050	Echelon I
0.005 lb	0.0054	Echelon I
0.003 lb	0.0044	Echelon I
0.002 lb	0.0045	Echelon I
0.001 lb	0.0012	Echelon I
8 oz	0.067	Echelon I
4 oz	0.037	Echelon I
2 oz	0.034	Echelon I
1 oz	0.0068	Echelon I

December 31, 2004

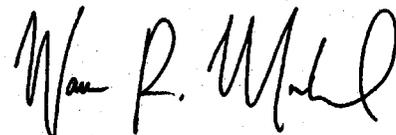

Effective through

For the National Institute of Standards and Technology

National Institute  
of Standards and Technology



National Voluntary  
Laboratory Accreditation Program

ISO/IEC 17025:1999  
ISO 9002:1994

## Scope of Accreditation



Revised 8/6/04

Page 5 of 5

### CALIBRATION LABORATORIES

NVLAP LAB CODE 200106-0

**DENVER INSTRUMENT COMPANY ALSO DOING BUSINESS AS SARTORIUS CORP.**

1/2 oz	0.0065	Echelon I
1/4 oz	0.0065	Echelon I
1/8 oz	0.0050	Echelon I
1/16 oz	0.0044	Echelon I
1/32 oz	0.0045	Echelon I
1/64 oz	0.0012	Echelon I

1. Represents an expanded uncertainty using a coverage factor,  $k=2$ .

December 31, 2004

Effective through

A handwritten signature in black ink, appearing to read 'William R. Mohr'. The signature is written in a cursive style.

For the National Institute of Standards and Technology