

National Institute
of Standards and Technology



National Voluntary
Laboratory Accreditation Program

ISO/IEC 17025:1999
ISO 9002:1994

Scope of Accreditation



Revised 4/26/04

Page 1 of 17

CALIBRATION LABORATORIES

NVLAP LAB CODE 200311-0

UNITED TESTING SYS. CANADA, LTD. DYNAMIC TESTING SYS. INT. INC.

225 Bradwick Drive, #21
Concord Ontario L4K 1K7
CANADA

Mr. Arno M. Dickertmann

Phone: 905-669-5327 Fax: 905-738-5051

E-Mail: arno@utscanada.com

URL: <http://www.utscanada.ccom>

NVLAP Code: 20/A01

ANSI/NCSL Z540-1-1994; Part 1

Compliant

DIMENSIONAL

NVLAP Code: 20/D05

Length

<i>Range</i>	<i>Best Uncertainty (\pm)^{note 1}</i>	<i>Remarks</i>
Extensometer Linear Calibrator		
0 to 25.4 mm (0 to 1.0 in)	0.33 μ m	ASTM E83
Extensometer Gage Length		
0 to 4.0 in	0.00137 in	ASTM E83
0 to 12.0 in	0.00177 in	ASTM E83

March 31, 2005

Effective through

For the National Institute of Standards and Technology

ISO/IEC 17025:1999
ISO 9002:1994

Scope of Accreditation



Revised 4/26/04

Page 2 of 17

CALIBRATION LABORATORIES

NVLAP LAB CODE 200311-0

UNITED TESTING SYS. CANADA, LTD. DYNAMIC TESTING SYS. INT. INC.

Crosshead Travel

0 to 24.0 in 0.00206 in Mitutoyo Digimatic

Field Service Calibration of Extensometers

0 to 1 in 0.000034 in ASTM E83

MECHANICAL

NVLAP Code: 20/M06
Force

	<i>Range in lbs</i>	<i>Best Uncertainty (\pm)^{note 1}</i>	<i>Remarks</i>
	0.1 to 112,404	0.025%	ASTM E74 ^{note 8}
	0.1 to 300,000	0.05%	ASTM E74 ^{note 8}
	0.1 to 1,000,000	0.25%	ASTM E4

Field Service Calibration of:

<i>Devices</i>	<i>Range in lbs</i>	<i>Best Uncertainty (\pm)^{note 1}</i>	<i>Remarks</i>
Tensile Testing Machines	to 1,000,000	0.25%	ASTM E4
Compression Testers	to 1,000,000	0.25%	ASTM E4

March 31, 2005

Effective through

For the National Institute of Standards and Technology



ISO/IEC 17025:1999
ISO 9002:1994

Scope of Accreditation



Revised 4/26/04

Page 3 of 17

CALIBRATION LABORATORIES

NVLAP LAB CODE 200311-0

UNITED TESTING SYS. CANADA, LTD. DYNAMIC TESTING SYS. INT. INC.

	<i>Range in Newton /Meter (Nm)</i>	<i>Best Uncertainty (±)^{note 1}</i>	<i>Remarks</i>
Torque	0.1 to 5000	0.05%	ASTM Z8494Z - Draft
Field Service Calibration:	0.1 to 5000	0.25%	ASTM Z8494Z - Draft

NVLAP Code: 20/M13

Field Service and Laboratory Calibration of Rockwell Hardness Testers- Indirect Hardness

	<i>Range in Rockwell Units</i>	<i>Best Uncertainty (±) in Rockwell Units^{notes 1,2}</i>
HRA	20 to 60	0.22
	60 to 80	0.12
	80 to 88	0.11
HRBS	20 to 50	1.01
	40 to 60	0.73
	60 to 70	0.46
HRC	20 to 40	0.39

March 31, 2005

Effective through

For the National Institute of Standards and Technology

ISO/IEC 17025:1999
ISO 9002:1994

Scope of Accreditation



Revised 4/26/04

Page 4 of 17

CALIBRATION LABORATORIES

NVLAP LAB CODE 200311-0

UNITED TESTING SYS. CANADA, LTD. DYNAMIC TESTING SYS. INT. INC.

	40 to 60	0.32
	60 to 70	0.31
HRC ^{note 3}	26.18	0.18
	45.43	0.17
	64.54	0.17
HRD	40 to 55	0.19
	55 to 65	0.21
	65 to 77	0.14
HRES	50 to 80	0.56
	80 to 90	0.56
	90 to 100	0.55
HRFS	60 to 70	0.46
	70 to 85	0.46
	85 to 100	0.45
HRGS	27 to 80	0.71
	80 to 94	0.24
HRHS	80 to 95	0.60


March 31, 2005

A handwritten signature in black ink, appearing to read "William R. Muhl".

Effective through

For the National Institute of Standards and Technology

National Institute
of Standards and Technology

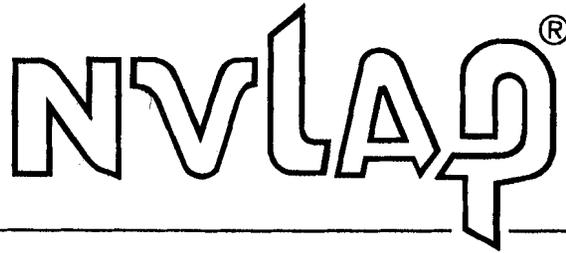

National Voluntary
Laboratory Accreditation Program

ISO/IEC 17025:1999
ISO 9002:1994

Scope of Accreditation



Revised 4/26/04

Page 5 of 17

CALIBRATION LABORATORIES

NVLAP LAB CODE 200311-0

UNITED TESTING SYS. CANADA, LTD. DYNAMIC TESTING SYS. INT. INC.

	95 to 100	0.39
HRKS	40 to 85	0.66
	85 to 100	0.63
HRLS	100 to 120	0.35
	120 to 130	0.35
HRMS	80 to 110	0.52
	110 to 130	0.48
HRPS	58 to 100	0.84
	100 to 112	0.51
HRRS	100 to 120	0.32
	120 to 127	0.20
HRSS	100 to 120	0.65
	120 to 125	0.14
HRVS	100 to 110	0.48
	110 to 121	0.17
HR15N	70 to 80	0.41
	80 to 90	0.20

March 31, 2005

Effective through

A handwritten signature in black ink, appearing to read 'William R. Muhl', is written over a horizontal line.

For the National Institute of Standards and Technology

National Institute
of Standards and Technology



National Voluntary
Laboratory Accreditation Program

ISO/IEC 17025:1999
ISO 9002:1994

Scope of Accreditation



Revised 4/26/04

Page 6 of 17

CALIBRATION LABORATORIES

NVLAP LAB CODE 200311-0

UNITED TESTING SYS. CANADA, LTD. DYNAMIC TESTING SYS. INT. INC.

	90 to 94	0.20
HR30B	42 to 60	0.40
	60 to 77.5	0.27
	77.5 to 86	0.27
HR45N	20 to 45	0.45
	45 to 66.5	0.45
	66.5 to 77	0.16
HR15TS	67 to 75	0.35
	75 to 85	0.35
	85 to 93	0.29
HR30TS	25 to 50	0.57
	50 to 70	0.72
	70 to 82	0.32
HR45TS	1 to 30	0.54
	30 to 50	0.67
	50 to 72	0.42
HR15WS	70 to 90	0.44

March 31, 2005

Effective through

A handwritten signature in black ink, appearing to read 'William R. Mohr', is written over a horizontal line.

For the National Institute of Standards and Technology

National Institute
of Standards and Technology



National Voluntary
Laboratory Accreditation Program

ISO/IEC 17025:1999
ISO 9002:1994

Scope of Accreditation



Revised 4/26/04

Page 7 of 17

CALIBRATION LABORATORIES

NVLAP LAB CODE 200311-0

UNITED TESTING SYS. CANADA, LTD. DYNAMIC TESTING SYS. INT. INC.

	90 to 100	0.54
HR30WS	60 to 80	0.80
	80 to 95	0.58
HR45WS	25 to 60	0.80
	60 to 95	0.94
HR15XS	80 to 90	0.56
	90 to 100	0.24
HR30XS	65 to 85	0.94
	85 to 100	0.14
HR45XS	50 to 85	0.70
	85 to 95	0.25
HR15YS	85 to 91	0.97
	91 to 96	0.96
	96 to 100	0.47
HR30YS	75 to 90	0.59
	90 to 100	0.32
HR45YS	65 to 85	0.68


March 31, 2005

Effective through

A handwritten signature in black ink, appearing to read 'William R. Muhl', is written over a horizontal line.

For the National Institute of Standards and Technology

National Institute
of Standards and Technology

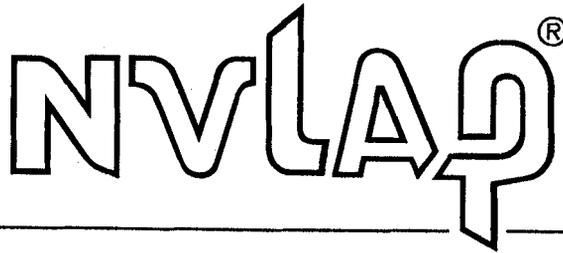

National Voluntary
Laboratory Accreditation Program

ISO/IEC 17025:1999
ISO 9002:1994

Scope of Accreditation



Revised 4/26/04

Page 8 of 17

CALIBRATION LABORATORIES

NVLAP LAB CODE 200311-0

UNITED TESTING SYS. CANADA, LTD. DYNAMIC TESTING SYS. INT. INC.

	85 to 100	0.24
Tungsten Carbide Balls		
HRBW	20 to 50	0.96
	50 to 75	0.65
	75 to 105	0.55
HREW	50 to 80	0.45
	80 to 90	0.50
	90 to 100	0.70
HRFW	60 to 70	0.55
	70 to 85	0.54
	85 to 100	0.55
HRGW	27 to 80	0.68
	80 to 94	0.18
HRHW	80 to 95	0.52
	95 to 100	0.42
HRKW	40 to 85	0.54

March 31, 2005

A handwritten signature in black ink, appearing to read 'William R. Muhl'.

Effective through

For the National Institute of Standards and Technology

ISO/IEC 17025:1999
ISO 9002:1994

Scope of Accreditation



Revised 4/26/04

Page 9 of 17


CALIBRATION LABORATORIES

NVLAP LAB CODE 200311-0

UNITED TESTING SYS. CANADA, LTD. DYNAMIC TESTING SYS. INT. INC.

	85 to 100	0.30
HRLW	100 to 120	0.17
	120 to 130	0.12
HRMW	80 to 110	0.53
	100 to 130	0.41
HRPW	58 to 100	0.56
	100 to 112	0.34
HRRW	100 to 120	0.28
	120 to 127	0.21
HRSW	100 to 120	0.78
	120 to 125	0.05
HRVW	100 to 110	0.25
	110 to 121	0.25
HR15TW	67 to 75	0.36
	75 to 85	0.24
	85 to 93	0.24
HR30TW	25 to 50	0.80

March 31, 2005

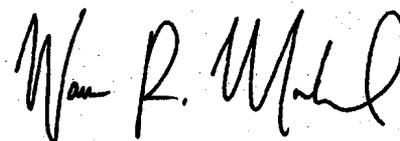

Effective through

For the National Institute of Standards and Technology

National Institute
of Standards and Technology



National Voluntary
Laboratory Accreditation Program

ISO/IEC 17025:1999
ISO 9002:1994

Scope of Accreditation



Revised 4/26/04

Page 10 of 17

CALIBRATION LABORATORIES

NVLAP LAB CODE 200311-0

UNITED TESTING SYS. CANADA, LTD. DYNAMIC TESTING SYS. INT. INC.

	50 to 70	0.47
	70 to 82	0.19
HR45TW	1 to 30	0.60
	30 to 50	0.36
	50 to 72	0.31
HR15WW	70 to 90	0.33
	90 to 100	0.33
HR30WW	60 to 95	0.40
HR45WW	25 to 60	0.75
	60 to 95	0.40
HR15XW	80 to 90	0.38
	90 to 100	0.10
HR30XW	65 to 85	0.83
	85 to 100	0.12
HR45XW	50 to 85	0.54
	85 to 95	0.11
HR15YW	85 to 91	0.32

March 31, 2005

A handwritten signature in black ink, appearing to read 'William R. Muhl'.

Effective through

For the National Institute of Standards and Technology

National Institute
of Standards and Technology



National Voluntary
Laboratory Accreditation Program

ISO/IEC 17025:1999
ISO 9002:1994

Scope of Accreditation



Revised 4/26/04

Page 11 of 17

CALIBRATION LABORATORIES

NVLAP LAB CODE 200311-0

UNITED TESTING SYS. CANADA, LTD. DYNAMIC TESTING SYS. INT. INC.

	91 to 96	0.15
	96 to 100	0.15
HR30YW	80 to 100	0.22
HR45YW	65 to 100	0.45

NVLAP Code: 20/M13

Field Service and Calibration of Rockwell Hardness Testers

	<i>Range</i>	<i>Best Uncertainty (\pm)^{note 1}</i>	<i>Remarks</i>
Force	3 kgf to 150 kgf	0.25%	ASTM E4 Direct verification of Force is applicable to all Rockwell Testers.
Depth	0 to 12 mm	0.0002 mm	Direct verification of Depth is limited to United True Blue II model hardness testers.

March 31, 2005

Effective through

For the National Institute of Standards and Technology

ISO/IEC 17025:1999
ISO 9002:1994

Scope of Accreditation



Revised 4/26/04

Page 12 of 17

CALIBRATION LABORATORIES

NVLAP LAB CODE 200311-0

UNITED TESTING SYS. CANADA, LTD. DYNAMIC TESTING SYS. INT. INC.


NVLAP Code: 20/M13

Field Service and Calibration of Macro Vickers Hardness Testers

Range 1 kgf to 30 kgf

<i>Load</i>	<i>Range (HV)</i>	<i>Best Uncertainty (HV)^{notes 1,5}</i>	<i>Remarks</i>
1 kgf	263	7.5	
1 kgf	457	15.8	
1 kgf	717	25.0	
5 kgf	263	6.3	
5 kgf	457	10.6	
5 kgf	717	11.2	
10 kgf	264	4.8	
10 kgf	443	5.5	
10 kgf	717	10.6	

March 31, 2005

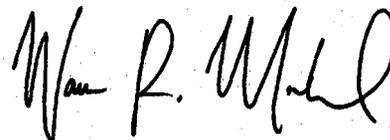

Effective through

For the National Institute of Standards and Technology

ISO/IEC 17025:1999
ISO 9002:1994

Scope of Accreditation



Revised 4/26/04

Page 13 of 17

CALIBRATION LABORATORIES

NVLAP LAB CODE 200311-0

UNITED TESTING SYS. CANADA, LTD. DYNAMIC TESTING SYS. INT. INC.

NVLAP Code: 20/M13

Field Service and Laboratory Calibration of Micro Hardness Testers - Indirect Method

Load Range 10 grams force to 1000 grams force

KNOOP SCALE ASTM 384


<i>Load</i>	<i>Range (HK)</i>	<i>Best Uncertainty (±)(HK)^{notes 1,6}</i>	<i>Remarks</i>
100 gf	95	5.9	
100 gf	600	21.5	
200 gf	95	5.3	
200 gf	523	16	
300 gf	95	4.7	
300 gf	600	16	
500 gf	95	3.2	
500 gf	600	20.8	
1000 g	600	15	

March 31, 2005

Effective through

For the National Institute of Standards and Technology

National Institute
of Standards and Technology

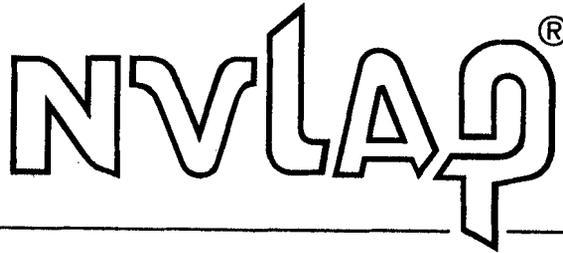

National Voluntary
Laboratory Accreditation Program

ISO/IEC 17025:1999
ISO 9002:1994

Scope of Accreditation



Revised 4/26/04

Page 14 of 17

CALIBRATION LABORATORIES

NVLAP LAB CODE 200311-0

UNITED TESTING SYS. CANADA, LTD. DYNAMIC TESTING SYS. INT. INC.

VICKERS SCALE ASTM E384

<i>Load</i>	<i>Range (HV)</i>	<i>Best Uncertainty (\pm)(HV)^{notes 1,6}</i>	<i>Remarks</i>
100 gf	96	6.8	
100 gf	541	15.1	
200 gf	95	5.3	
200 gf	523	9.9	
300 gf	95	4.7	
300 gf	554	18.5	
500 gf	95	5.0	
500 gf	553	21.1	
1000 gf	94	3.3	
1000 gf	555	17.4	

March 31, 2005

A handwritten signature in black ink, appearing to read 'William R. Mohr', is written over a horizontal line.

Effective through

For the National Institute of Standards and Technology

ISO/IEC 17025:1999
ISO 9002:1994

Scope of Accreditation



Revised 4/26/04

Page 15 of 17

CALIBRATION LABORATORIES

NVLAP LAB CODE 200311-0

UNITED TESTING SYS. CANADA, LTD. DYNAMIC TESTING SYS. INT. INC.

NVLAP Code: 20/M13

Field Service and Laboratory Calibration of Brinell Hardness Testers

	<i>Range (ABW)</i>	<i>Best Uncertainty (±)(HBW)^{note 1}</i>	<i>Remarks</i>
Force	3 kgf to 150 kgf	0.25%	ASTM E4
Indentation Measuring System	0 to 7 mm	0.0008 mm	
Ball Measuring System	10 mm	0.0005 mm	

NVLAP Code: 20/M13

Field Service and Laboratory Calibration of Brinell Hardness Testers

Range 500 kgf to 3000 kgf

<i>Load</i>	<i>Range (HBW)</i>	<i>Best Uncertainty (±)(HBW)^{notes 1,7}</i>	<i>Remarks</i>
500 kgf	15.0 to 100.0	3.8	
500 kgf	100.0 to 158.0	4.1	
3000 kgf	100.0 to 200.0	3.8	
3000 kgf	200.0 to 400.0	5.3	
3000 kgf	400.0 to 600.0	5.3	

March 31, 2005

Effective through

For the National Institute of Standards and Technology

Scope of Accreditation



Revised 4/26/04

Page 16 of 17

CALIBRATION LABORATORIES

NVLAP LAB CODE 200311-0

UNITED TESTING SYS. CANADA, LTD. DYNAMIC TESTING SYS. INT. INC.

1. Represents an expanded uncertainty using a coverage factor, $k=2$.
2. The HRC standardized test blocks used for verification are calibrated at the David Ellis Company Inc. Hardness Calibration Laboratory in accordance with ASTM E18 section C using NIST Rockwell HRC standards reference materials (SRM) 2810, 2811, and 2812. All other Rockwell Scales are traceable to David L. Ellis Co. Inc. hardness levels through laboratory standardizing machines. The standardizing machines are directly verified according to ASTM E18 using devices that are traceable to NIST.
3. Scale are Rockwell HRC SRM'S 2810, 2811, and 2812 purchased from NIST and maintained by UTS/DTS.
4. The standardized test blocks used for verification are calibrated at the David Ellis Company Inc. Hardness Calibration Laboratory in accordance with ASTM E18 Section C. Rockwell Scales are traceable to David L. Ellis Co. Inc. hardness levels through laboratory standardizing machines. The standardizing machines are directly verified according to ASTM E18 using devices that are traceable to NIST.
5. The standardized test blocks used for verification are calibrated in accordance with ASTM E92 using Indenter / load combinations that are traceable to D.L. Ellis Co. hardness levels, through laboratory standardizing machines. The standardizing machines are directly verified according to ASTM E92 using devices to NIST.
6. The standardized test blocks used for verification are calibrated in accordance with ASTM E384 using Indenter / load combinations that are traceable to D.L. Ellis Co. hardness levels, through laboratory standardizing machines. The standardizing machines are directly verified according to ASTM E384 using devices that are traceable to NIST.
7. The standardized test blocks used for verification are calibrated in accordance with ASTM E10 using Indenter / load combinations that are traceable to D.L. Ellis Co. hardness levels,

March 31, 2005

A handwritten signature in black ink, appearing to read "William R. Miller".

Effective through

For the National Institute of Standards and Technology

National Institute
of Standards and Technology



National Voluntary
Laboratory Accreditation Program

ISO/IEC 17025:1999
ISO 9002:1994

Scope of Accreditation



Revised 4/26/04

Page 17 of 17

CALIBRATION LABORATORIES

NVLAP LAB CODE 200311-0

UNITED TESTING SYS. CANADA, LTD. DYNAMIC TESTING SYS. INT. INC.

through laboratory standardizing machines. The standardizing machines are directly verified according to ASTM E10 using devices that are traceable to NIST.

8. Different uncertainties are available depending upon which standards is used. Please contact the laboratory for more information.

March 31, 2005

A handwritten signature in black ink, appearing to read 'William R. Muhl'.

Effective through

For the National Institute of Standards and Technology